

AD-A055 928

H S S INC BEDFORD MASS

F/G 17/5

DEVELOPMENT OF A HIGH-RESOLUTION IMAGE INTENSIFIED SPECTROGRAPH--ETC(U)

APR 77 A H TUTTLE

DNA001-76-C-0097

UNCLASSIFIED

HSS-R-032


DNA-440AF

NI

| OF |  
AD  
A055 928



END  
DATE  
FILMED  
8 -78  
DDC

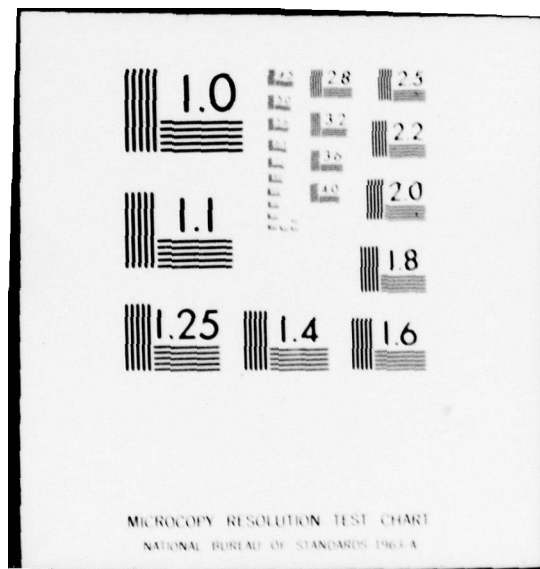

FOR FURTHER TRAN

AD-E300225

DNA 4408F

SBLE AD-E300225

AD A 055928

# DEVELOPMENT OF A HIGH-RESOLUTION IMAGE INTENSIFIED SPECTROGRAPH.

HSS Incorporated  
2 Alfred Circle  
Bedford, Massachusetts 01730

A. H. Tuttle

19 Apr 1977

HSS-B-032

22 p.

Final Report 10 Nov 1975-30 Apr 1977

CONTRACT No. DNA 001-76-C-0097

APPROVED FOR PUBLIC RELEASE;  
DISTRIBUTION UNLIMITED.

THIS WORK SPONSORED BY THE DEFENSE NUCLEAR AGENCY  
UNDER RDT&E RMSS CODE B322076462 K43AAXHX68413 H2590D.

AD No. 1  
DDC FILE COPY

Prepared for  
Director  
DEFENSE NUCLEAR AGENCY  
Washington, D. C. 20305

DDC  
RECEIVED  
JUL 5 1978  
B

390 794

# UNCLASSIFIED

SECURITY CLASSIFICATION OF THIS PAGE (When Data Entered)

REPORT DOCUMENTATION PAGE		READ INSTRUCTIONS BEFORE COMPLETING FORM
1. REPORT NUMBER <b>DNA 4408F</b>	2. GOVT ACCESSION NO.	3. RECIPIENT'S CATALOG NUMBER
4. TITLE (and Subtitle) <b>DEVELOPMENT OF A HIGH-RESOLUTION IMAGE INTENSIFIED SPECTROGRAPH</b>	5. TYPE OF REPORT & PERIOD COVERED <b>Final Report for Period 10 Nov 75-30 Apr 77</b>	
7. AUTHOR(s) <b>A. H. Tuttle</b>	6. PERFORMING ORG. REPORT NUMBER <b>HSS-B-032</b>	
9. PERFORMING ORGANIZATION NAME AND ADDRESS <b>HSS Incorporated 2 Alfred Circle Bedford, Massachusetts 01730</b>	8. CONTRACT OR GRANT NUMBER(s) <b>DNA 001-76-C-0097</b> <i>new</i>	
11. CONTROLLING OFFICE NAME AND ADDRESS <b>Director Defense Nuclear Agency Washington, D.C. 20305</b>	10. PROGRAM ELEMENT, PROJECT, TASK AREA & WORK UNIT NUMBERS <b>NWET Subtask K43AAXHX684-13</b>	
14. MONITORING AGENCY NAME & ADDRESS (if different from Controlling Office)	12. REPORT DATE <b>19 April 1977</b>	
	13. NUMBER OF PAGES <b>28</b>	
	15. SECURITY CLASS (of this report) <b>UNCLASSIFIED</b>	
16. DISTRIBUTION STATEMENT (of this Report)  <b>Approved for public release; distribution unlimited.</b>		
17. DISTRIBUTION STATEMENT (of the abstract entered in Block 20, if different from Report)		
18. SUPPLEMENTARY NOTES  <b>This work sponsored by the Defense Nuclear Agency under RDT&amp;E RMSS Code B322076462 K43AAXHX68413 H2590D.</b>		
19. KEY WORDS (Continue on reverse side if necessary and identify by block number) <b>Image Intensified High Resolution Cross Dispersed Echelle Spectrograph Contact Film Recording on Fiber-Optic Output Screen</b>		
20. ABSTRACT (Continue on reverse side if necessary and identify by block number) <b>This instrument was developed to provide high resolution spectral information of low light level optical radiation from atomic and molecular species related to the infrared chemistry of the upper atmos- phere when excited by electron bombardment from a rocket-borne electron accelerator.</b>		

UNCLASSIFIED

SECURITY CLASSIFICATION OF THIS PAGE (When Data Entered)



## TABLE OF CONTENTS

<u>Section</u>	<u>Page</u>
1. INTRODUCTION	3
2. BACKGROUND	4
3. INSTRUMENT DESIGN GOALS	7
4. INSTRUMENT FINAL CHARACTERISTICS	8
5. INSTRUMENT OPTICAL COMPONENTS, PARAMETERS AND CHARACTERISTICS	9
5.1 OPTICAL	9
5.2 SPECTRAL	9
5.3 SPECTRAL WAVELENGTH ORDERS	10
6. MECHANICAL CHARACTERISTICS	11
7. ELECTRICAL CHARACTERISTICS	13
8. FINAL TEST RESULTS	14
8.1 FIGURE AND PHOTOGRAPH COMMENTS	14

## LIST OF ILLUSTRATIONS

<u>Figure</u>	<u>Legend</u>	<u>Page</u>
1.	Optical Diagram of Spectrograph.	15
2.	Photograph displaying inherent pincushion distortion of a 3-stage electrostatically focused image intensifier.	17
3.	Photograph of Iron Spectrum with transparent overlay of pincushion grid.	18
4.	Photograph of the complete spectrograph.	19
5.	Photograph of the instrument with covers removed.	20
6.	Close-up photograph of electrical control panel.	21

BY		
DISTRIBUTION/AVAILABILITY CODES		
Date:      /      /      or SPECIAL		
A		

## DEVELOPMENT OF A HIGH RESOLUTION IMAGE INTENSIFIED SPECTROGRAPH

### 1. INTRODUCTION

This instrument was developed to provide high resolution spectral information of low light level radiations from atomic and molecular species related to the IR chemistry of the upper atmosphere when excited by electron bombardment by a rocket-borne electron accelerator.

A near-optimum instrument has been developed under this contract to provide a diagnostic tool to record visible-radiating species related to the IR chemistry of the metastable state of atomic nitrogen,  $N(^2D)$ , and atomic oxygen  $O(^1S)$  and  $O(^1D)$  in the altitude range of 90-120 kms. The instrument combines several state-of-the-art design features; i. e., fast F/number, echelle and crossed dispersion gratings, image intensification, and direct photographic film contact with the fiber-optic output screen of an image intensifier. The combination of these design features increases the total sensitivity of this instrument far in excess of any spectrograph used for collecting this type of spectral information on Exceed-type programs.

PRECEDING PAGE BLANK

## 2. BACKGROUND

In 1974, operating under contract to Utah State University and AFCRL, HSS Inc developed an image-intensified spectrograph named Cygnus for use on Project Precede. The Precede event, sponsored by DNA, had as its principle objective the test of the performance of a rocket-borne electron accelerator in the altitude range of 90-120 kilometers. Ground based optical measurements, including the use of the Cygnus spectrograph, were performed as an aid to diagnosing the accelerator performance, as back-up to the payload photometers, and as an evaluation of techniques for making ground based measurements of electron-induced atmospheric processes.

The results of the Precede Event, conducted at White Sands Missile Range on 17 October 1974, demonstrated incontrovertibly the importance of ground based measurements to upper atmospheric aeronomy programs involving electron deposition. In the Precede case, for example, a malfunction of the system for removing the covers of the on-board photometers rendered those instruments, in effect, inoperative and the only data obtained was from the ground based instruments.

The Cygnus spectrograph obtained data over the entire operating period of the electron-accelerator. The data was of good quality but was contaminated by an unexpected source of light, as was the data from the other ground based instruments. The contaminating light source was related to unspent propellant emanating from the combustion chamber of the second stage booster which was deliberately left attached to the accelerator payload to improve vehicle neutralization.

Cygnus spectrograph is a low-dispersion survey-type instrument covering the wavelength region from  $4200 \text{ \AA}$  to  $8500 \text{ \AA}$ . The large



wavelength coverage is perhaps its greatest attribute. Its wavelength resolution, spatial resolution and sensitivity are modest. Size, weight, and configuration of the instrument are such that the instrument lends itself to easy adaptation to any kind of automatic or manually trainable mount.

The Cygnus instrument with its low dispersion,  $220 \text{ \AA}^\circ$  per millimeter, and consequent modest resolution,  $10 \text{ to } 12 \text{ \AA}^\circ$ , is a suitable instrument for certain classes of measurements on Exceed type programs. It is the equivalent of 400 photometer channels each  $10 \text{ \AA}^\circ$  wide, albeit of reduced sensitivity. With it, prominent features of the spectrum can be readily observed and their temporal and to some degree spatial features can be studied.

The goal of Exceed type events is the study of atmospheric chemistry processes in the vicinity of altitudes around 100 kilometers under controlled conditions of electron impact. The complex chemistry chains that result from this electron deposition must be understood for many upper atmospheric problems and applications.

The optical spectra induced by the chemical processes are primarily infrared radiations and weak visible or near-visible radiations. In a low resolution instrument such as Cygnus and in photometers, these weak visible radiations tend to be swamped by the radiations of neighboring prominent atomic lines or molecular bands. One is thus led to conclude that to improve upon present ground based spectral measurements better wavelength resolution is required.

Perhaps one of the most important visible-radiating species related to the IR chemistry is the metastable state of atomic nitrogen,  $N(^2D)$ . Consequently, any consideration of new or improved instrumentation should provide for the capability of recording this atomic doublet. The previous instrument CYGNUS did not have the sensitivity to record  $N(^2D)$

emissions from any planned EXCEED event even if it had sufficient spectral resolution to isolate it from adjacent spectral features.

The requirement for improved sensitivity alone did not justify a completely new instrument. Improvements could have been made to the existing Cygnus which would have increased its sensitivity and thereby improved its performance and capabilities. However, the requirement for increased wavelength resolution, an increase of between a factor of 10 or 20, could only have been fulfilled by a completely new approach to the spectral dispersion system, making a new instrument approach mandatory.

The new instrument Super Cygnus combines both high resolution and increased sensitivity to provide an instrument with far more capability for providing spectral information related to the IR chemistry problems. In addition, it has improved spatial resolution another limitation of the Cygnus instrument.



### 3. INSTRUMENT DESIGN GOALS

The optical, mechanical, and electrical design of the Super Cygnus spectrograph was designed in accordance with good commercial practices. The design goals of the instrument are as follows:

<u>Parameter</u>	<u>Design Goal</u>
Wavelength Coverage . . . . .	4200 Å - 7500 Å
Linear Dispersion . . . . .	15 Å/mm
Wavelength Resolution . . . . .	1 Å
Relative Aperture . . . . .	f/1.5
Field of View (variable) . . . . .	0.5 - 2.0 degrees
Image Intensifier . . . . .	3 stage electrostatic
Radiant Power Gain . . . . .	40,000
Cathode Response . . . . .	S-20 VR
Phosphor Screen . . . . .	P-11
Film Size . . . . .	70 mm
Exposure Times (Optional) . . . . .	1, 2, 5, 10, 20 sec

#### 4. INSTRUMENT FINAL CHARACTERISTICS

The instrument final characteristics are better than the design goals in two major respects. The image intensifier has a higher radiant power gain and using a reflective cross dispersion grating instead of a transmission type allowed us to have more grooves per millimeter thus larger separation between spectral orders and linear dispersions from  $14 \text{ \AA/mm}$  to  $25 \text{ \AA/mm}$ .

<u>Parameter</u>	<u>Final Characteristics</u>
Wavelength Coverage . . . . .	$4200 \text{ \AA} - 7500 \text{ \AA}$
Linear Dispersion . . . . .	$14 \text{ \AA/mm} - 25 \text{ \AA/mm}$
Wavelength Resolution . . . . .	$1 \text{ \AA}$
Relative Aperture . . . . .	$f/1.5$
Field of View (variable) . . . . .	$0.5 - 2.0$ degrees
Image Intensifier . . . . .	3 stage electrostatic
Radiant Power Gain . . . . .	75,000
Cathode Response . . . . .	S-20 VR
Phosphor Screen . . . . .	P-11
Film Size . . . . .	70 mm x 125 ft
Exposure Times (Optional) . . . . .	1, 2, 5, 10, 20 sec.

## 5. INSTRUMENT OPTICAL COMPONENTS, PARAMETERS AND CHARACTERISTICS

### 5.1 Optical

<u>Parameter</u>	<u>Specification</u>
Objective Lens . . . . .	Modified Maksutov Catadioptric 300 mm FL., F/3.0 w/field flattener lens.
Collimator Lens . . . . .	Schneider Xenotar Lens 150 mm FL, F/2.8.
Camera Lens . . . . .	Farrand Optical Co. Super Farron Lens w/IRIS 76 mm FL, F/0.87
Operating F/No. . . . .	F/1.5
Image Intensifier Tube . . . . .	VARO Inc Type 8606, 40mm dia. Cathode, 3 stage inten- sification w/fiber optic ex- tension on anode screen, w/P-11 Phosphor.
Magnification . . . . .	0.9
Radiant Power Gain . . . . .	75,000
Field of View (variable) . . . . .	0.5 - 2.0 degrees

### 5.2 Spectral

Configuration . . . . .	Cross dispersing system. Echelle Grating for high resolution and plane reflec- tion grating for order sorting.
Dispersion Grating . . . . .	Echelle grating, Bausch and Lomb Type 35-03-25-401 79 Grooves/mm. 63°26' blaze angle.
Order Sorting Grating . . . . .	Plane reflectance grating. Bausch and Lomb Type 35-53-20-280, 1200 grooves/ mm. 17°27' blaze angle.

### 5.3 SPECTRAL WAVELENGTH ORDERS

Total wavelength coverage . . . . . 4200 Å - 7500 Å  
 Linear dispersion . . . . . 14 Å/mm - 25 Å/mm  
 Wavelength Resolution . . . . . 1 Å  
 Orders . . . . . 30-52

Spectral Order	Wavelength Coverage (Å)	Linear (Å/mm) Dispersion	Wavelength Resolution (Å)
30	7220 to 7720	24.8	0.99
31	6990 to 7460	24.0	0.96
32	6750 to 7220	23.3	0.93
33	6580 to 6990	22.5	0.90
34	6390 to 6780	21.9	0.88
35	6220 to 6580	21.3	0.85
36	6050 to 6390	20.7	0.83
37	5890 to 6220	20.1	0.80
38	5740 to 6050	19.6	0.78
39	5590 to 5890	19.1	0.76
40	5460 to 5440	18.6	0.74
41	5330 to 5590	18.1	0.72
42	5200 to 5460	17.7	0.70
43	5090 to 5330	17.3	0.69
44	4970 to 5200	16.9	0.68
45	4870 to 5090	16.5	0.66
46	4760 to 4970	16.2	0.65
47	4660 to 4870	15.8	0.63
48	4570 to 4760	15.5	0.62
49	4480 to 4660	15.2	0.60
50	4390 to 4570	14.9	0.59
51	4300 to 4480	14.6	0.58
52	4220 to 4390	14.3	0.57



## 6. MECHANICAL CHARACTERISTICS

Film Transport . . . . .	70 mm film movement enclosed in a light tight case painted reflective white, with a reciprocating film pressure platen for providing direct contact of the film with the image intensifier fiber optic output face plate screen.
Film Transport Rates . . . . .	The film transport is operated with a camera programmer Model CC-384X. The spectrograph incorporates an internal shutter which is synchronized with the film movement. It operates in a normally open to open mode, closing only when the film is advanced. The choice of film rates are 1 picture per second, 1 every 2 seconds, 1 every 5 seconds, 1 every 10 seconds, and 1 every 20 seconds.
Shutter (capping) . . . . .	A 2 inch diameter HARVARD shutter is incorporated in the optical path to cap the input light to the image intensifier during film transportation. It is synchronized with the film transport and camera control unit.
Spectrograph . . . . .	All of the optical and mechanical components are mounted to a common frame and base plate which is enclosed with a light tight cover painted reflective white with access hatches, one to change slits or field of view limiters and one to adjust the camera lens focus for extreme temperature compensation.
Grating Holders . . . . .	Both gratings are mounted in front surface pivoted adjustable, goniometric grating mounts.



Weight . . . . .	157 pounds
Mounting points . . . . .	The spectrograph has two optional mounting configurations. One is for "in laboratory use", three adjustable leveling pads are arranged on an 18-inch per leg triangle pattern attached to the bottom of the instrument base plate. The other method of mounting is for "in field use" on a tracking mount rail. When this is required, an interface plate with two shoes attached is bolted to the three threaded bases that normally hold the "in laboratory use" leveling pads. These shoes in turn bolt to the tracking mount instrument rail.
Center of Gravity . . . . .	The center of gravity is indicated in three axes on the instrument with CG decals.

## 7. ELECTRICAL CHARACTERISTICS

All electrical functions are controlled by an electrical switch panel with lights to indicate all functions. (see Fig. 6, pg 20)

<u>Item</u>	<u>Function</u>
Film Transport . . . . .	Switch Position Up = Automatic (Programed) Center = OFF, Momentary Down = Manual Film Advance.
Image Intensifier . . . . .	On-Off = 6.75 VDC Battery Power.
AC Power . . . . .	On-Off = 115 VAC Power to Film Transport and Capping Shutter.
Shutter Disable . . . . .	Up = Normally Open, Light Off. Down = Closed, Light On, indicating that the shutter is disabled and in the capping mode.
Electrical Connector and Camera Cable . . . . .	Control Power to Film Transport.
Electrical Connector 115 VAC . . . . .	Power for control circuit to film transport and shutter.
Electrical Connector Programmer . . . . .	Signals for exposure rates to film transport and shutter are supplied by a Model CC-384X camera programmer.

## 8. FINAL TEST RESULTS.

The contracting officer's representative, Mr. William Isengard, visited HSS Inc laboratory on the week of 19 October 1976. At that time we conducted final optical alignment of the optical components and permanently bolted these components in place. The system was operated and spectral sources were photographed on film. A Nikon camera was used to photograph the Image Intensifier output because the film transport enclosure was not completely fabricated at that time. Resolution and dispersion tests were conducted and evaluated. The instrument either met or surpassed all of the design goals and was tentatively accepted by Mr. Isengard pending a final integrated test incorporating the film transport coupled to the image intensifier fiber-optic output screen with the electrical control circuit in full operation.

The film transport was completed in mid November 1976. The spectrograph was electrically wired and the switch and relay control panel was installed and tested.

The film transport was tested with film in direct contact with the Image Intensifier output fiber optic screen and spectrums were photographed of several spectral sources.

The results were excellent; there were no static electric charge problems with the film in direct contact with the fiber optic face plate or in transport. The entire instrument system operated very satisfactorily.

The high resolution image intensified spectrograph is completed and Final Acceptance by the contracting officer was conducted on April 21 and 22, 1977.

### 8.1 Figure and Photograph Comments.

Figure 1 is a diagramatic layout in plan view of the instrument identifying the location of all the principal components of the spectrograph.

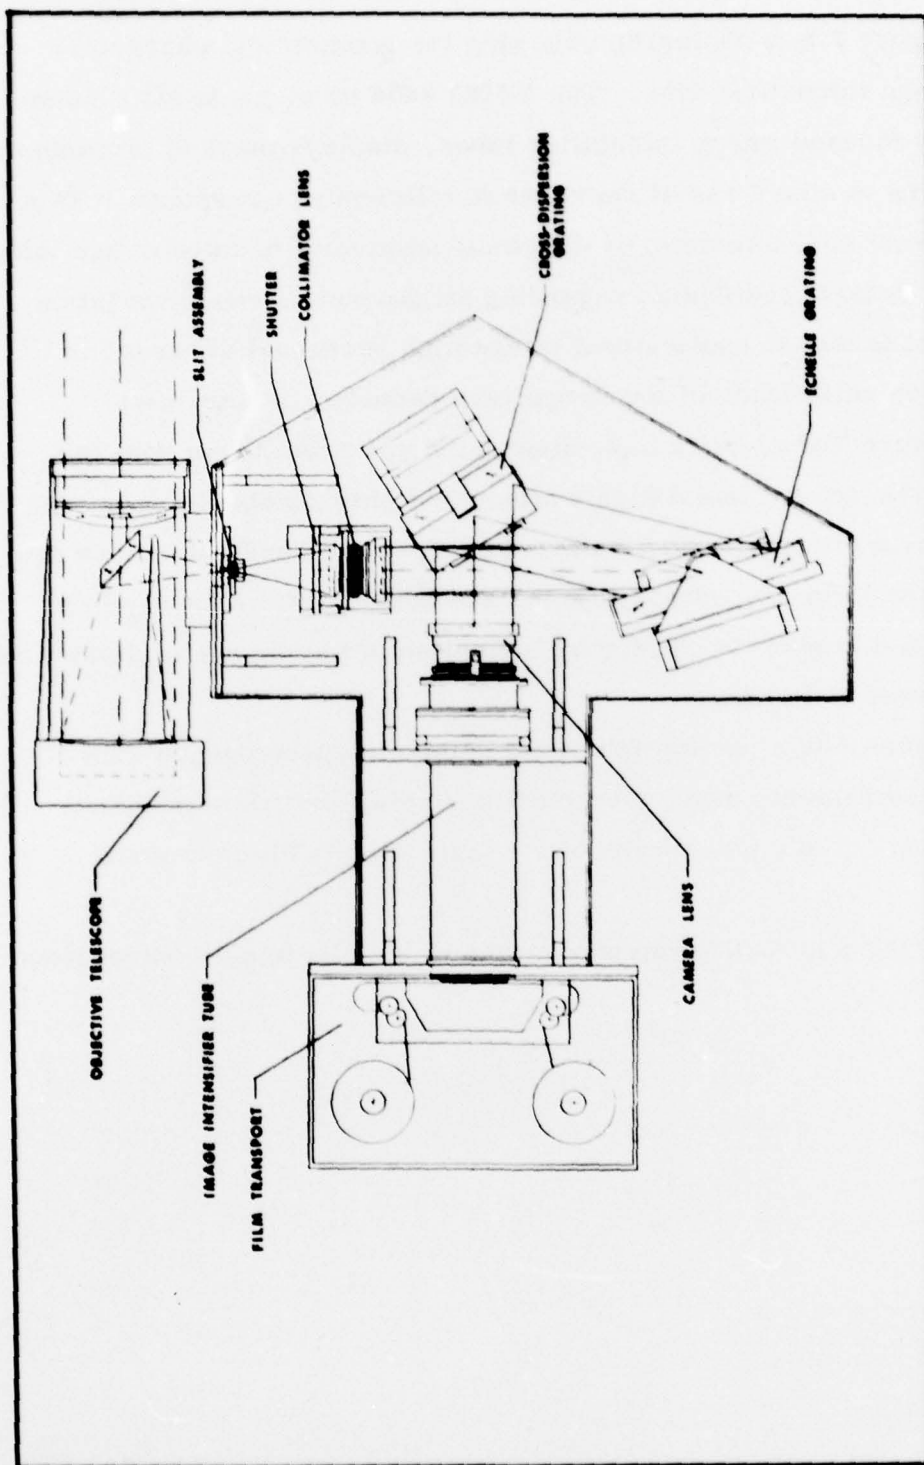


Figure 1. Optical Diagram of Spectrograph.



Figure 2 is a photograph showing the geometrical characteristics of the image intensifier tube. The VARO 8606 tube, as do all 3-stage electrostatically focused image intensifier tubes, displays marked pincushion distortion. There is also a radial decrease in efficiency of response. This again is an inherent characteristic of the electrostatically focused image intensifier tubes. A general conclusion regarding all geometric characteristics of the instrument is that in applications where high positional accuracy is required, detailed calibration of the image tube geometry is essential.

Figure 3 presents a high-dispersion spectrum taken with the spectrograph. The source was a highly attenuated glow discharge spectrum of iron excited by a microwave generator. Twenty-three spectral orders are covered by the spectrogram, although some are quite faint. A transparent overlay is provided to give the reader an indication of the degree of distortion present in each spectral order.

Figure 4 is a photograph of the complete spectrograph with objective lens, instrument cover, electrical controls, and film transport.

Figure 5 is a photograph of the instrument with the covers removed.

Figure 6 is a close-up photograph of the electrical control panel.



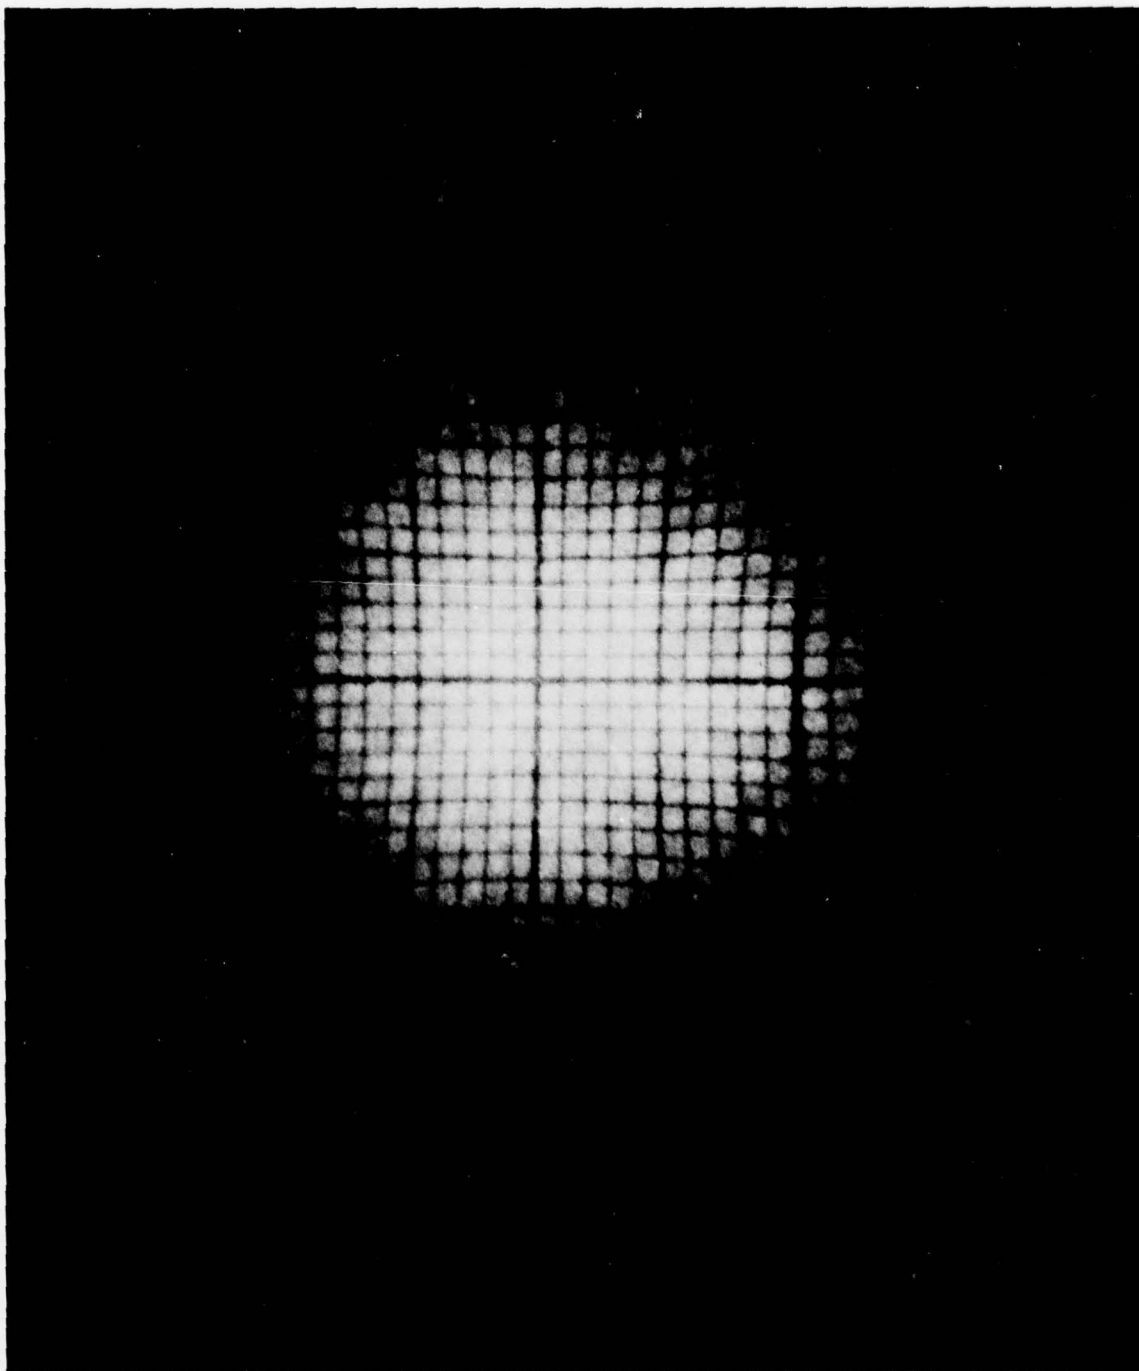


Figure 2. Photograph of rectangular grid placed on face of image intensifier tube.

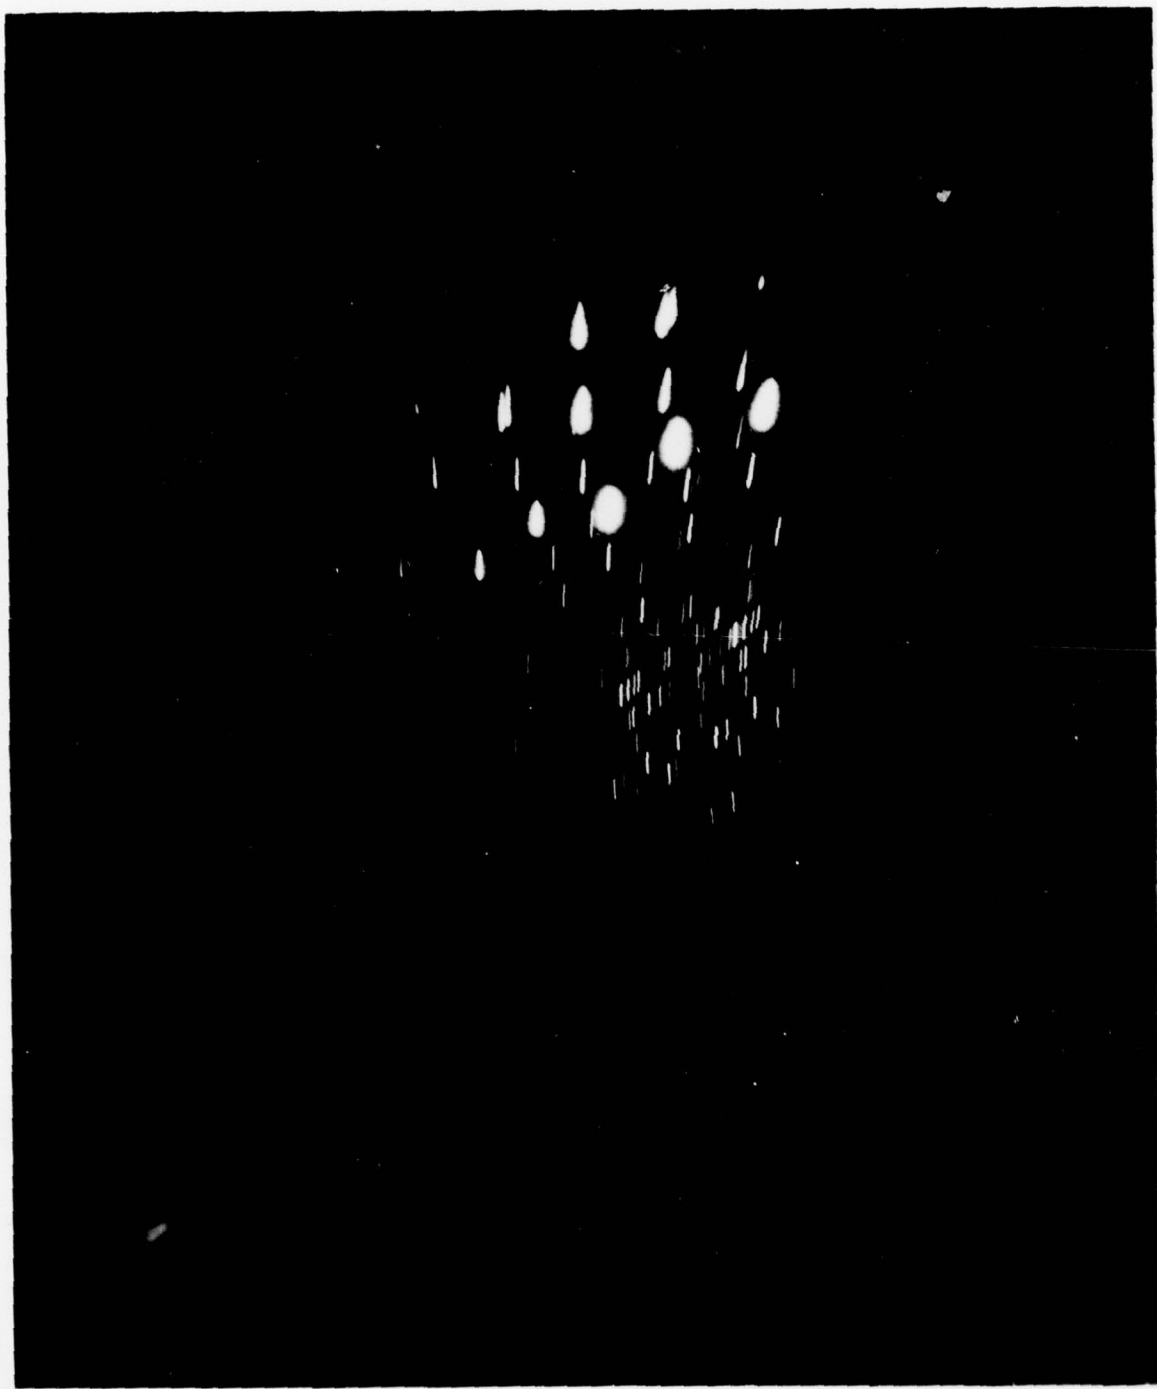


Figure 3. Spectrogram of Iron glow-discharge source with transparent overlay of pincushion distortion grid.

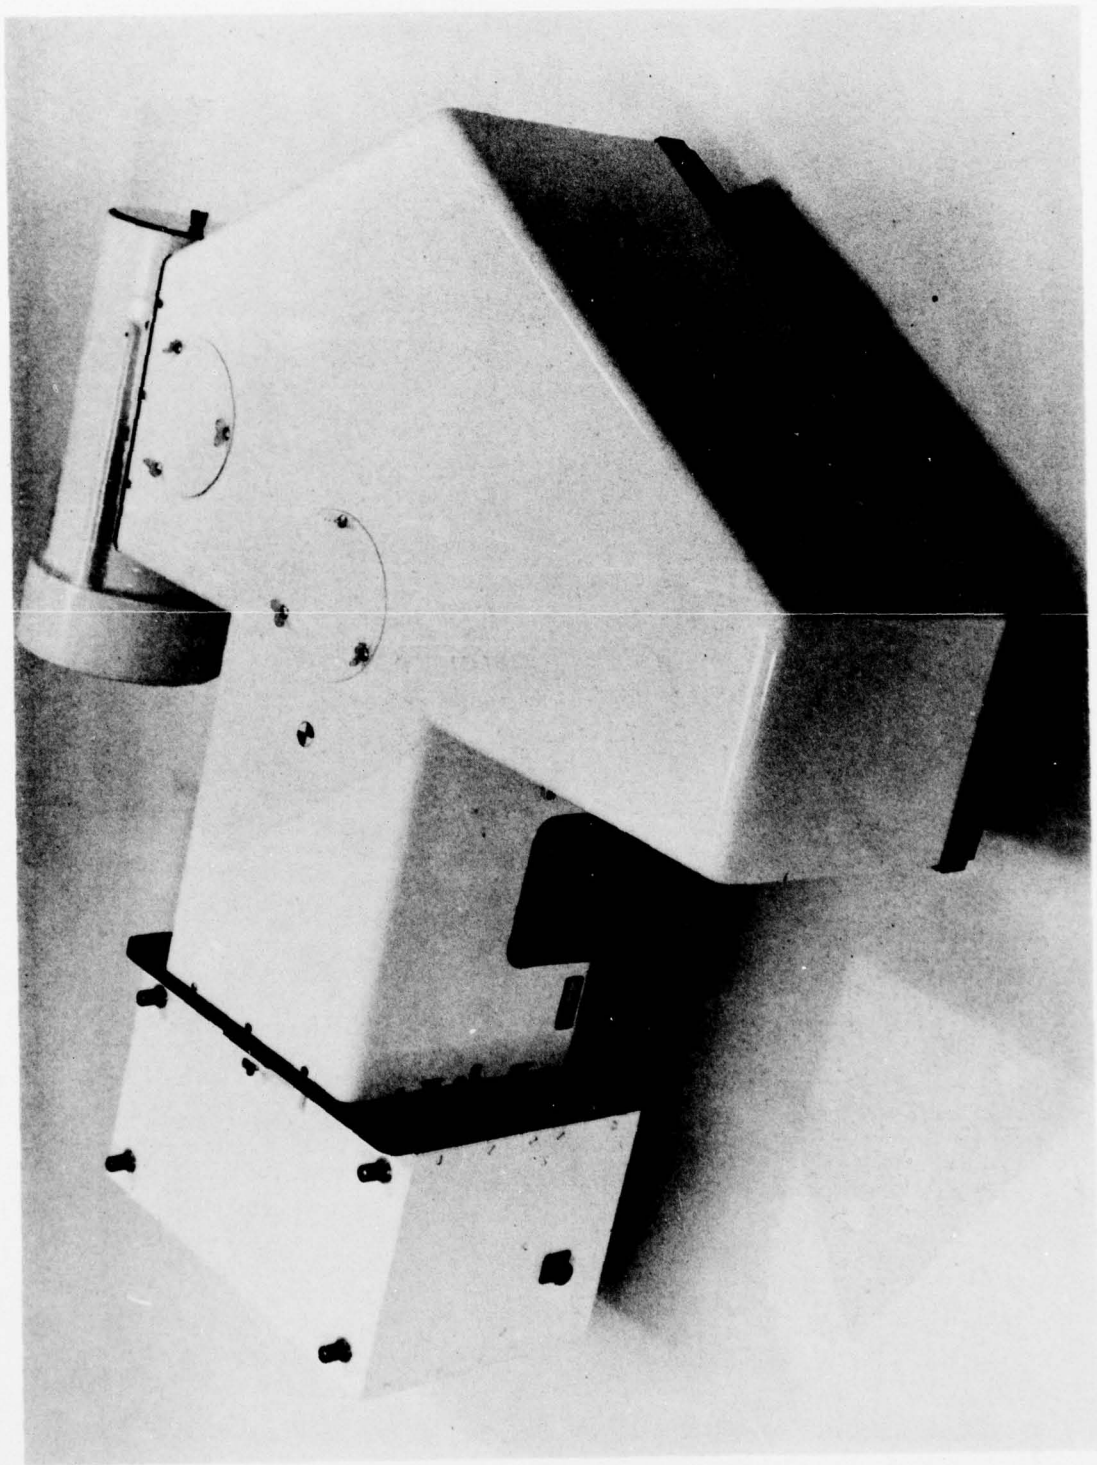


Figure 4. Completed Super Cygnus Spectrograph.

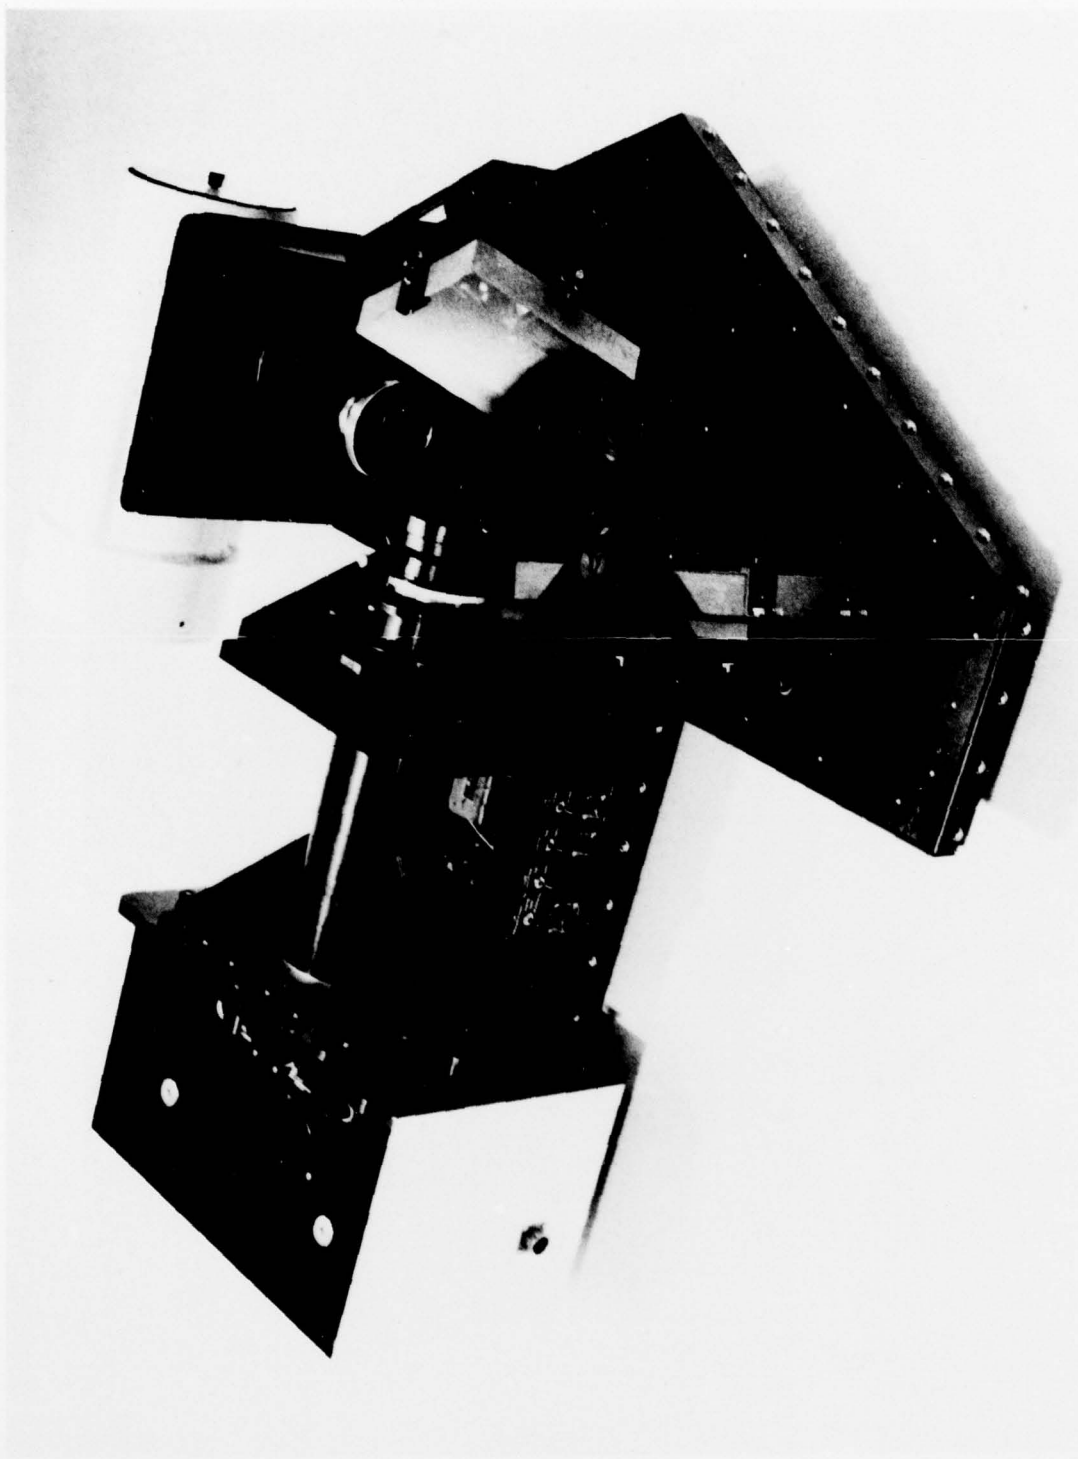


Figure 5. Super Cygnus with instrument covers removed.

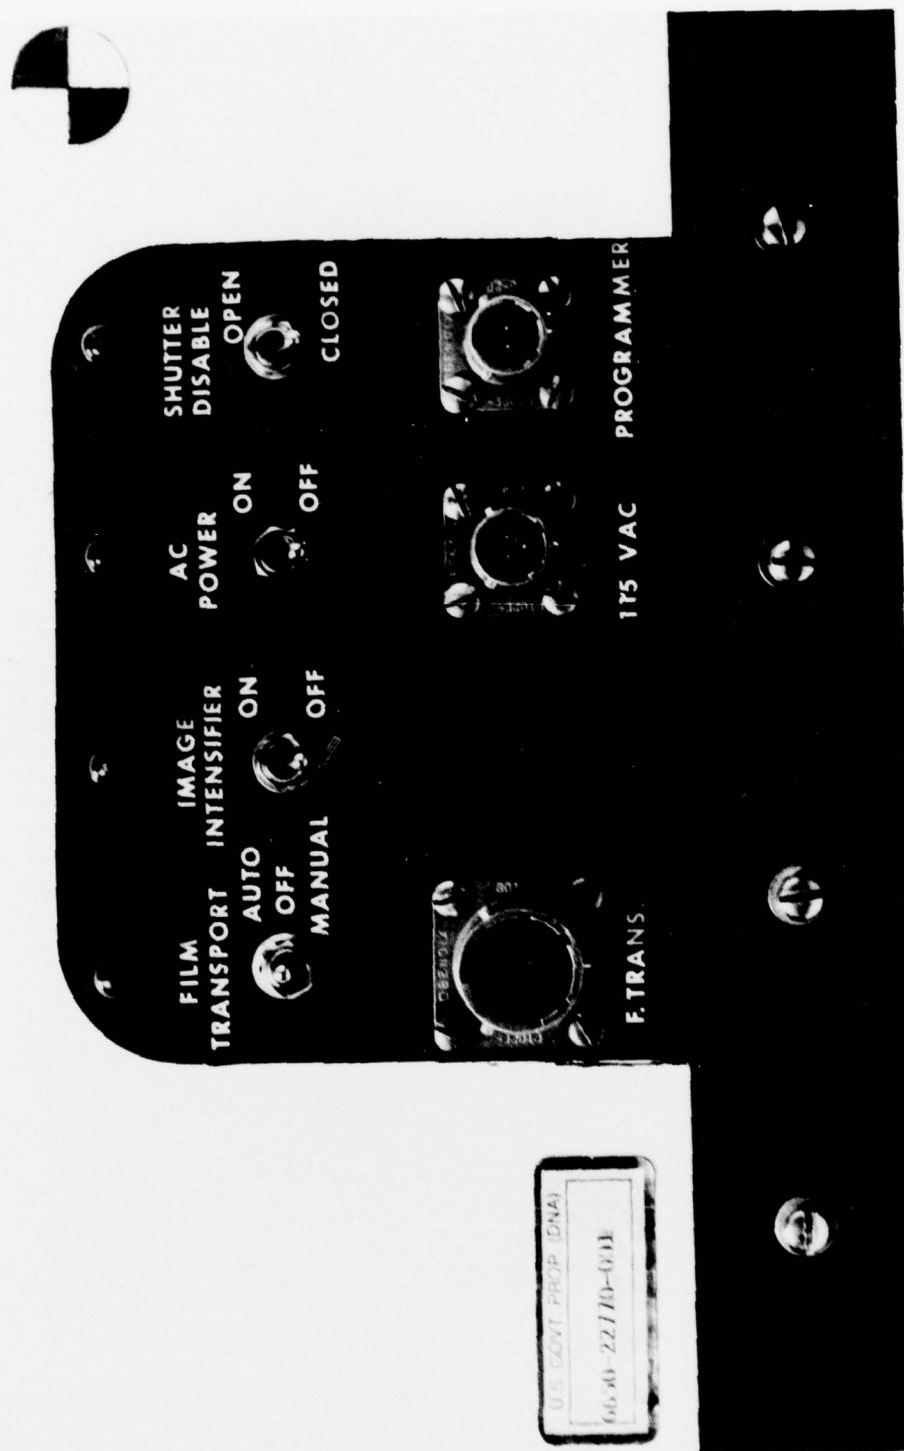


Figure 5. Close-up of electrical control panel.



## DISTRIBUTION LIST

### DEPARTMENT OF DEFENSE

Director  
Defense Advanced Rsch. Proj. Agency  
ATTN: LTC W. A. Whitaker  
ATTN: Strategic Technology Office  
ATTN: Nuclear Monitoring Research

Defense Documentation Center  
Cameron Station  
12 cy ATTN: TC

Director Defense Nuclear Agency  
ATTN: TISI Archives  
ATTN: RAAE, MAJ John Clark  
ATTN: RAEV, Harold C. Fitz, Jr.  
ATTN: DDST  
ATTN: RAAE, MAJ James W. Mayo  
3 cy ATTN: TITL, Tech. Lib.  
2 cy ATTN: RAAE, Charles A. Blank

Commander  
Field Command  
Defense Nuclear Agency  
ATTN: FCPR

Chief  
Livermore Division, Fld. Command DNA  
Lawrence Livermore Laboratory  
ATTN: FCPRL

Under Secy. of Def. for Rsch. & Engrg.  
ATTN: S&SS(OS)

### DEPARTMENT OF THE ARMY

Commander/Director  
Atmospheric Sciences Laboratory  
U.S. Army Electronics Command  
ATTN: DELAS-AE-M, F. E. Niles  
ATTN: H. Ballard  
ATTN: DRSEL-BL-SY-S, D. Snider  
ATTN: R. Rosen

Commander  
Harry Diamond Laboratories  
2 cy ATTN: DELHD-NP, F. N. Wimenitz

Commander  
U.S. Army Nuclear Agency  
ATTN: MONA-WE, J. Berberet

Director  
BMD Advanced Tech. Center  
ATTN: ATC-O, W. Davies  
ATTN: ATC-T, Melvin T. Capps

Dep. Chief of Staff for Rsch. Dev. & Acq.  
ATTN: NCB Division  
ATTN: DAMA-CSZ-C  
ATTN: Dama-WSZ-C

Chief of Engineers  
ATTN: Fernand DePersin

### DEPARTMENT OF THE ARMY (Continued)

Dep. Chief of Staff for Ops. & Plans  
ATTN: DAMO-DDL, COL D. W. Einsel  
ATTN: Div. of Chem. & Nuc. Ops.

Director  
U.S. Army Ballistic Research Labs.  
ATTN: Tech. Lib., E. Baicy  
ATTN: John Mester  
ATTN: J. Heimerl  
ATTN: M. Kregl

Commander  
U.S. Army Electronics Command  
ATTN: DRSEL-PL-ENV, Hans A. Bomke  
ATTN: DRSEL  
ATTN: Stanley Kronenberg  
ATTN: DRSEL-RD-P  
ATTN: DRSEL-TL-IR, E. T. Hunter  
ATTN: Inst. for Exploratory Rsch.  
ATTN: Weapons Effects Section

Commander  
U.S. Army Foreign Science & Tech. Ctr.  
ATTN: Robert Jones

Commander  
U.S. Army Material Dev. & Rdns. Cmd.  
ATTN: DRXCD-TL  
ATTN: DRCCDC, J. A. Bender

Commander  
U.S. Army Missile Command  
ATTN: DRSMI-ABL  
ATTN: Chief, Doc. Section  
ATTN: DRSMI-XS, Chief Scientist

Chief  
U.S. Army Research Office  
ATTN: CRDARD-CCS, Hermann Robl  
ATTN: CRDARD-P, Robert Mace

### DEPARTMENT OF THE NAVY

Chief of Naval Research  
ATTN: Code 421, B. R. Junker  
ATTN: Code 461, Jacob Warner  
ATTN: Code 461, R. G. Joiner

Commander  
Naval Ocean Systems Center  
ATTN: Code 2200 1, Verne E. Hildebrand  
ATTN: Code 2200, Ilan Rothmuller  
ATTN: Code 2200, Jurgan Richter  
ATTN: Code 2200, William F. Moler  
ATTN: Code 2200, Richard Pappert  
ATTN: Tech. Lib. for T. J. Keary  
ATTN: Code 2200, Herbert Hughes

Superintendent (Code 1424)  
Naval Postgraduate School  
ATTN: Code 2124, Tech. Reports Librarian

DEPARTMENT OF THE NAVY (Continued)

Director

Naval Research Laboratory

ATTN: Douglas P. McMutt  
ATTN: Code 7701, Jack D. Brown  
ATTN: Code 7709, Wahab Ali  
ATTN: Code 7750, Darrell F. Strobel  
ATTN: Code 7700, Timothy P. Coffey  
ATTN: Code 7750, Paul Julienne  
ATTN: Code 2600, Tech. Lib.  
ATTN: Code 7127, Charles Y. Johnson  
ATTN: Code 7120, W. Neil Johnson  
ATTN: Code 7750, J. Davis  
ATTN: Code 7750, Klaus Hein  
ATTN: Code 7750, Joel Feddler  
ATTN: Code 2027, Tech. Lib.  
ATTN: Code 7750, S. L. Ossakow  
ATTN: Code 7730, Edgar S. McClean

Officer-in-Charge

Naval Surface Weapons Center

ATTN: Code WA501, Navy Nuc. Prgms. Off.  
ATTN: Code WX21, Tech. Lib.  
ATTN: D. J. Sand  
ATTN: L. Rudlin

Commanding Officer

Naval Intelligence Support Center

ATTN: Doc. Con.  
ATTN: Code 40A, E. Blase

Commander

Naval Weather Service Command

ATTN: Mr. Martin

DEPARTMENT OF THE AIR FORCE

AF Geophysics Laboratory, AFSC

5 cy ATTN: OPR, Alva T. Stair  
5 cy ATTN: LKB, Kenneth S. W. Champion  
2 cy ATTN: OPR-1, R. Murphy  
2 cy ATTN: OPR-1, J. Kennealy  
5 cy ATTN: OPR, J. Ullwick

AF Weapons Laboratory, AFSC

ATTN: CA  
ATTN: Col G. J. Freyer  
2 cy ATTN: DYM  
5 cy ATTN: DYC  
5 cy ATTN: SUL  
5 cy ATTN: DYT

Commander

ASD

ATTN: ASD-YH-EX, Lt Col Robert Leverette

SAMSO/SZ

ATTN: SZJ, Maj Lawrence Doan

AFTAC

5 cy ATTN: TD  
2 cy ATTN: Tech. Lib.

Hq. USAF

ATTN: DLS  
ATTN: DLCAW  
ATTN: DTL  
ATTN: DLXP  
ATTN: SDR  
ATTN: Tech. Lib.

DEPARTMENT OF THE AIR FORCE (Continued)

SAMSO/AW

ATTN: AW

DEPARTMENT OF ENERGY

Division of Military Application

ATTN: Doc. Con. for Major D. A. Haycock  
ATTN: Doc. Con. for Colonel T. Gross  
ATTN: Doc. Con. for David Slade  
ATTN: Doc. Con. for Donald I. Gale  
ATTN: Doc. Con. for F. S. Ross

Los Alamos Scientific Laboratory

ATTN: Doc. Con. for R. A. Jeffries  
ATTN: Doc. Con. for C. R. Mehl  
ATTN: Doc. Con. for G. Rood  
ATTN: Doc. Con. for H. V. Sego  
ATTN: Doc. Con. for D. Steinhaus  
ATTN: Doc. Con. for J. Judd  
ATTN: Doc. Con. for T. Bieniewski  
ATTN: Doc. Con. for D. M. Rohrer  
ATTN: Doc. Con. for Martin Tierney  
ATTN: Doc. Con. for Marge Johnson  
ATTN: Doc. Con. for John S. Malik  
ATTN: Doc. Con. for William Maier  
ATTN: Doc. Con. for S. Rockwood  
ATTN: Doc. Con. for Donald Kerr  
ATTN: Doc. Con. for W. D. Barfield  
ATTN: Doc. Con. for Reference Library  
ATTN: Doc. Con. for W. M. Hughes  
ATTN: Doc. Con. for E. W. Jones, Jr.  
ATTN: Doc. Con. for John Zinn  
ATTN: Doc. Con. for E. S. Bryant

University of California

Lawrence Livermore Laboratory

ATTN: G. R. Haugen  
ATTN: A. Kaufman  
ATTN: D. J. Wuebbles  
ATTN: J. F. Tinney  
ATTN: Julius Chang  
ATTN: Tech. Info. Dept.  
ATTN: W. H. Duerwer

Sandia Laboratories

ATTN: Doc. Con. for W. D. Brown  
ATTN: Doc. Con. for Org. 9220  
ATTN: Doc. Con. for Craig Hudson  
ATTN: Doc. Con. for J. C. Eckardt  
ATTN: Doc. Con. for C. W. Gwyn  
ATTN: Doc. Con. for D. A. Dahlgren  
ATTN: Doc. Con. for M. L. Kramm  
ATTN: Doc. Con. for T. Wright  
ATTN: Doc. Con. for Charles Williams  
ATTN: Doc. Con. for Sandia Rpt. Coll.  
ATTN: Doc. Con. for Doc. Con. Div.

Sandia Laboratories

Livermore Laboratory

ATTN: Doc. Con. for Thomas Cook

Department of Energy

Div. of Hqs. Services, Library Branch, G-043

ATTN: Doc. Con. for D. Kohlstedt  
ATTN: Doc. Con. for J. D. LaFleur  
ATTN: Doc. Con. for Class. Tech. Lib.  
ATTN: Doc. Con. for George Regosa  
ATTN: Doc. Con. for Rpts. Section  
ATTN: Doc. Con. for R. Kandel  
ATTN: Doc. Con. for H. H. Kurzweg

DEPARTMENT OF ENERGY (Continued)

Argonne National Laboratory

Records Control

ATTN: Doc. Con. for A. C. Wall  
ATTN: Doc. Con. for S. Gabelnick  
ATTN: Doc. Con. for J. Berkowitz  
ATTN: Doc. Con. for Lib. Svcs. Rpts. Sec.  
ATTN: Doc. Con. for Len Liebowitz  
ATTN: Doc. Con. for David W. Green  
ATTN: Doc. Con. for Gerald T. Reedy

OTHER GOVERNMENT AGENCY

Department of Commerce  
Office of Telecommunications  
Institute for Telecom Science  
ATTN: William F. Utlaut

DEPARTMENT OF DEFENSE CONTRACTORS

Aero-Chem Research Laboratories, Inc.

3 cy ATTN: A. Fontijn

Aerodyne Research, Inc.

ATTN: M. Camac  
ATTN: F. Bien

Aerospace Corporation

ATTN: Harris Mayer  
ATTN: Thomas D. Taylor  
ATTN: R. D. Rawcliffe  
ATTN: R. Grove  
ATTN: R. J. McNeal

University of Denver

Colorado Seminary

Denver Research Institute

ATTN: Sec. Officer for Mr. Van Zyl  
ATTN: Sec. Officer for David Murcray

General Electric Company

TEMPO-Center for Advanced Studies

ATTN: Warren S. Knapp  
5 cy ATTN: DASIAC, Art Feryok

General Research Corporation

ATTN: John Ise, Jr.

Geophysical Institute

University of Alaska

ATTN: T. N. Davis  
3 cy ATTN: Neal Brown

Honeywell Incorporated

Radiation Center

ATTN: W. Williamson

HSS Incorporated

ATTN: A. H. Tuttle

Institute for Defense Analyses

ATTN: Hans Wolfhard  
ATTN: Ernest Bauer

DEPARTMENT OF DEFENSE CONTRACTORS (Continued)

Lockheed Missiles and Space Co. Inc.

ATTN: Billy M. McCormac, Dept. 52-54  
ATTN: John B. Cladis, Dept. 52-12  
ATTN: J. B. Reagan, Dept. 52-12  
ATTN: John Kumer  
ATTN: Martin Walt, Dept. 52-10  
ATTN: Richard G. Johnson, Dept. 52-12  
ATTN: Robert D. Sears, Dept. 52-14  
ATTN: Tom James

Mission Research Corporation

ATTN: P. Fischer  
ATTN: D. Archer

Photometrics, Inc.

3 cy ATTN: I. L. Kofsky/D. P. Villanucci/G. Davidson

Physical Dynamics, Inc.

ATTN: Joseph B. Workman

Physical Sciences, Inc.

ATTN: Kurt Wray

R & D Associates

ATTN: Robert E. Lelevier  
ATTN: Forrest Gilmore

R & D Associates

ATTN: Herbert J. Mitchell

Science Applications, Inc.

ATTN: Daniel A. Hamlin

Space Data Corporation

ATTN: Edward F. Allen

SRI International

ATTN: M. Baron  
ATTN: Ray L. Leadabrand  
ATTN: Walter G. Chesnut

SRI International

ATTN: Warren W. Berning

Technology International Corporation

ATTN: W. P. Boquist

Utah State University

ATTN: D. Burt  
ATTN: Kay Baker  
ATTN: C. Wyatt  
ATTN: Doran Baker

Visidyne, Inc.

ATTN: L. Katz  
ATTN: Wil iam Reidy  
ATTN: Henry J. Smith  
ATTN: Charles Humphrey  
ATTN: J. W. Carpenter  
ATTN: T. C. Degges